
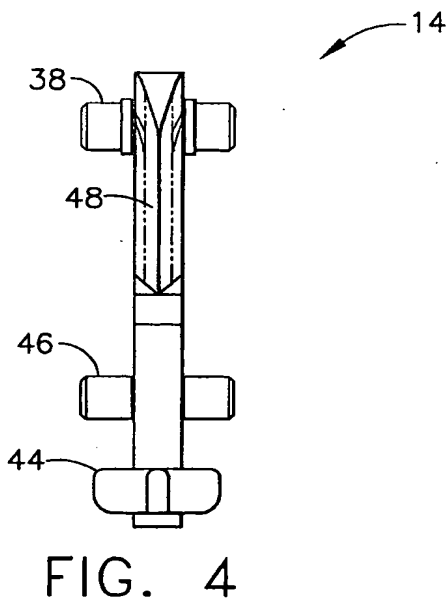


2/27

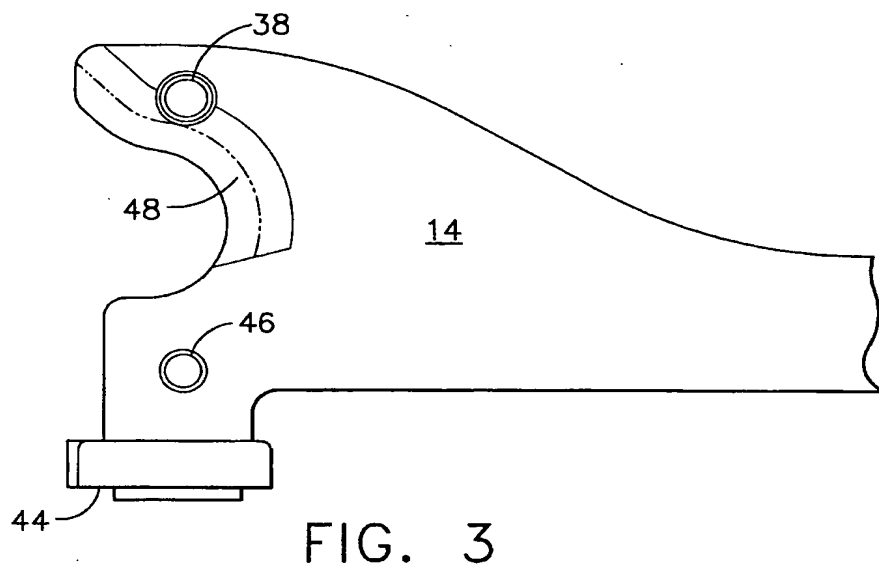

Title: Surgical Stapling Instrument Having a Lockout  
Mechanism for Prevention of Firing  
Inventor: Kevin Doll et al.  
**Docket: END-887CIP**  
ATTY: Dean L. Garner: Phone: (513) 337-8559

3/27

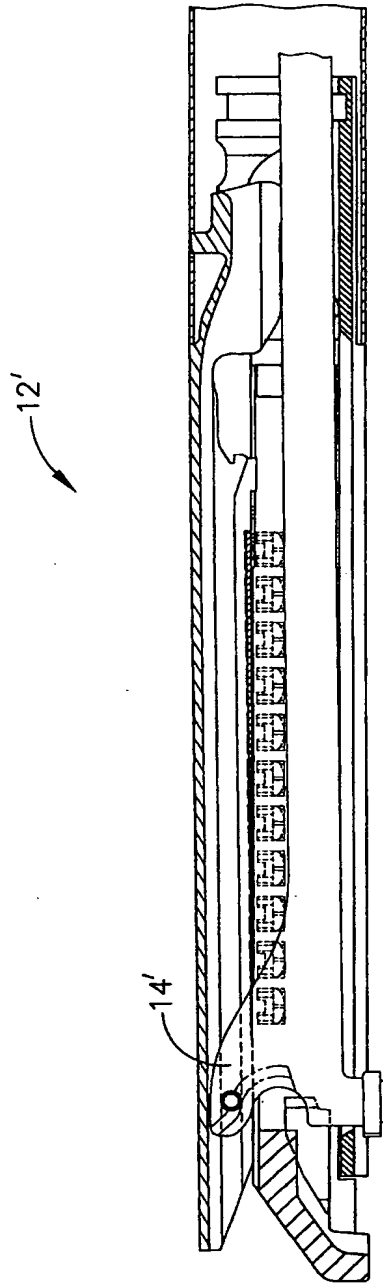


FIG. 5

4/27


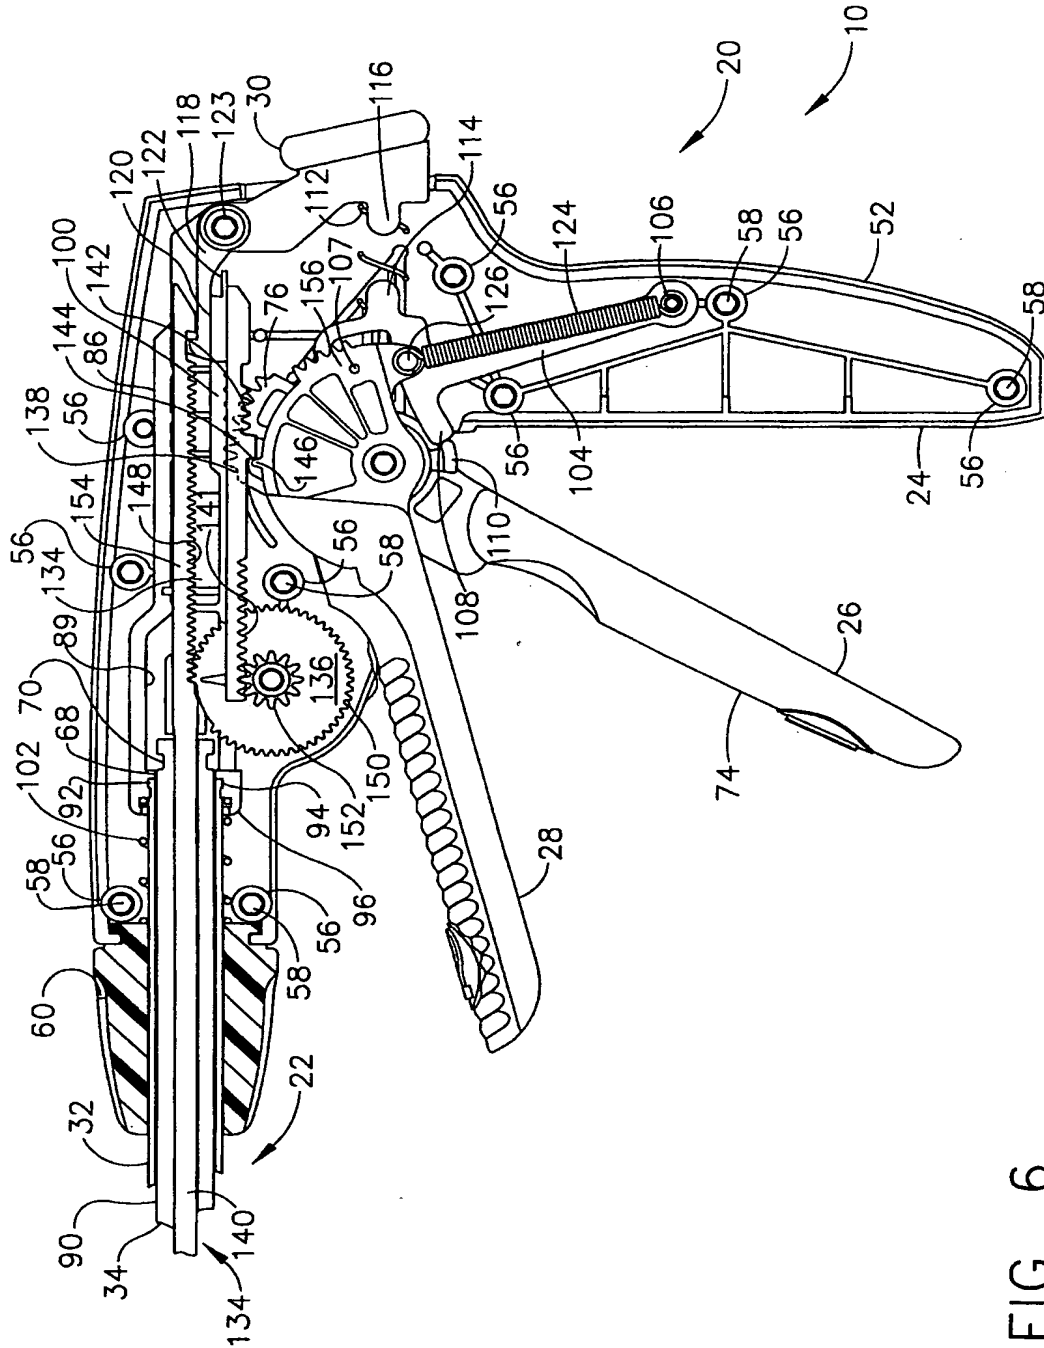


FIG. 6

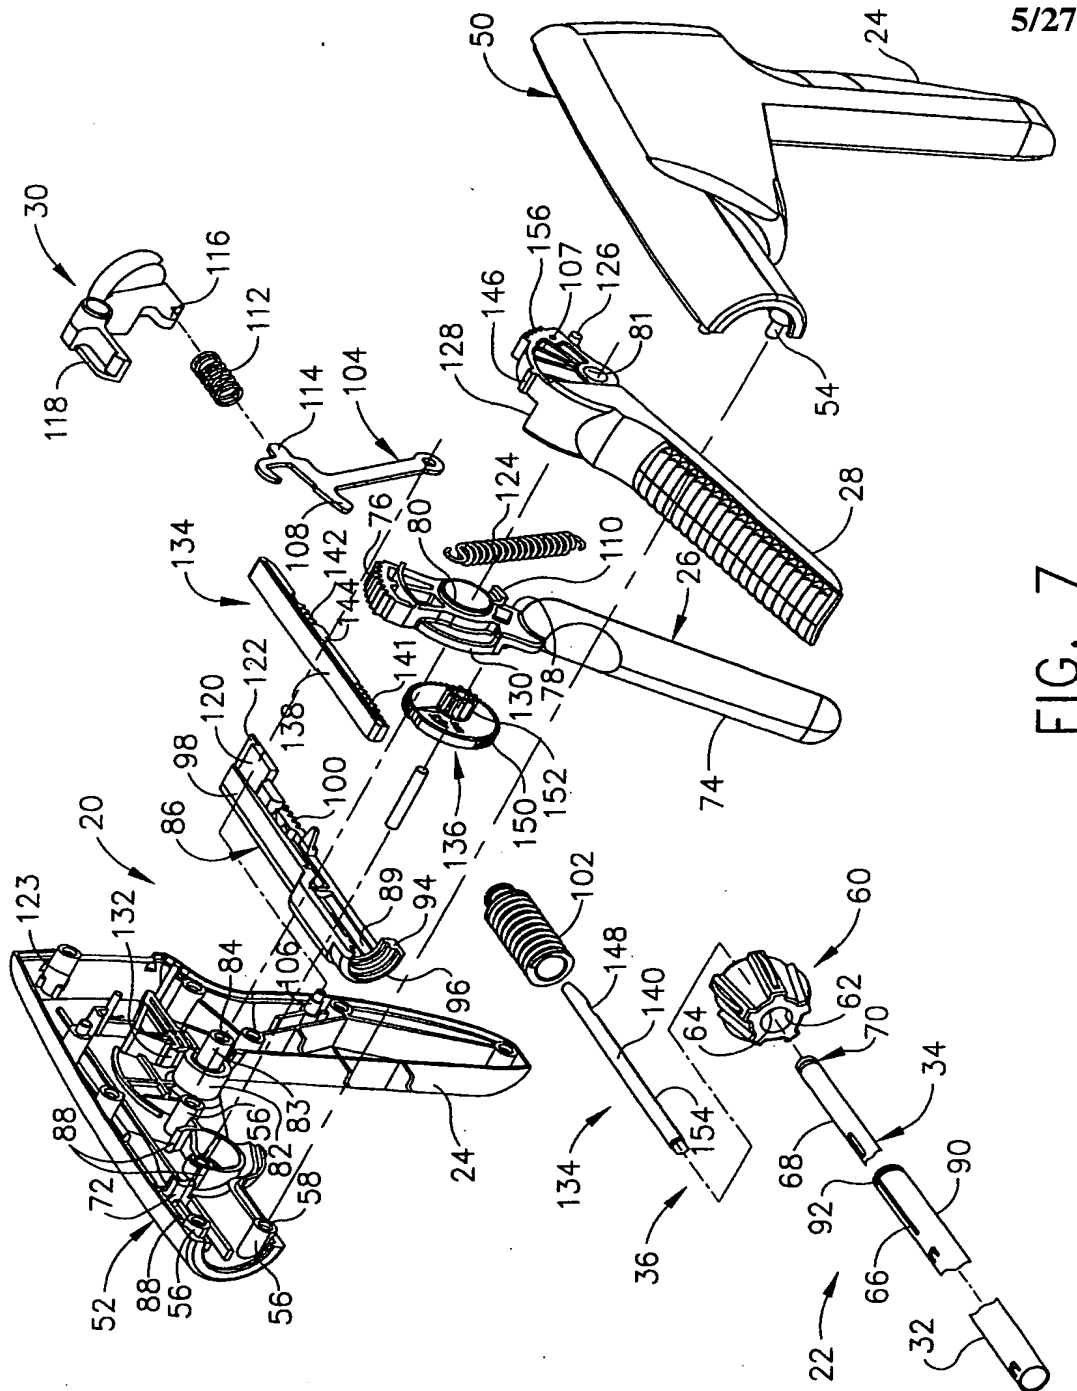

6/27

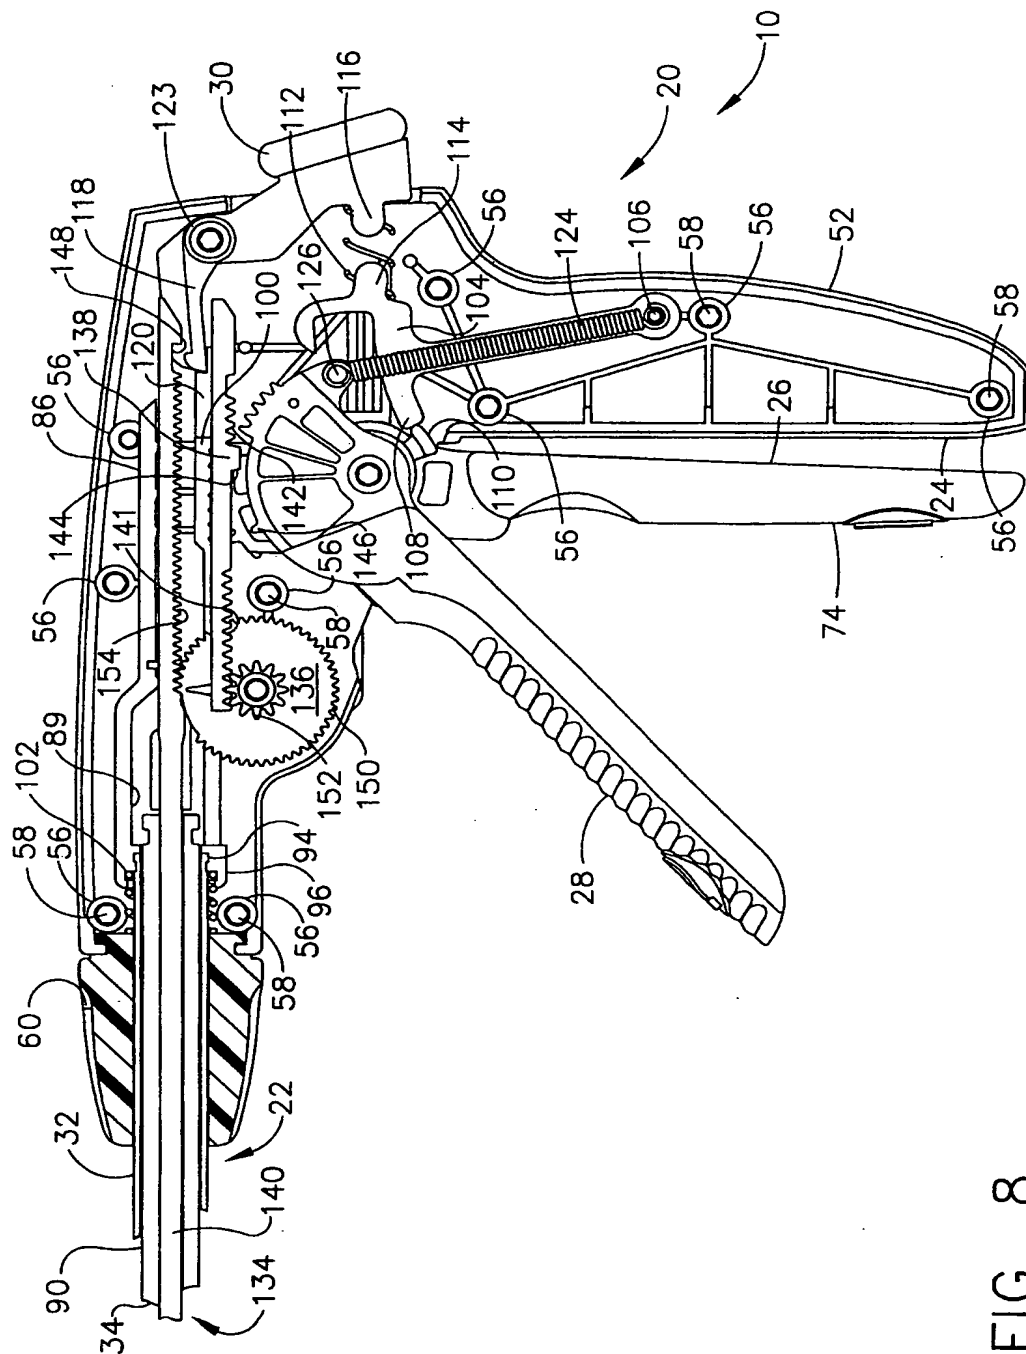


FIG. 8

7/27


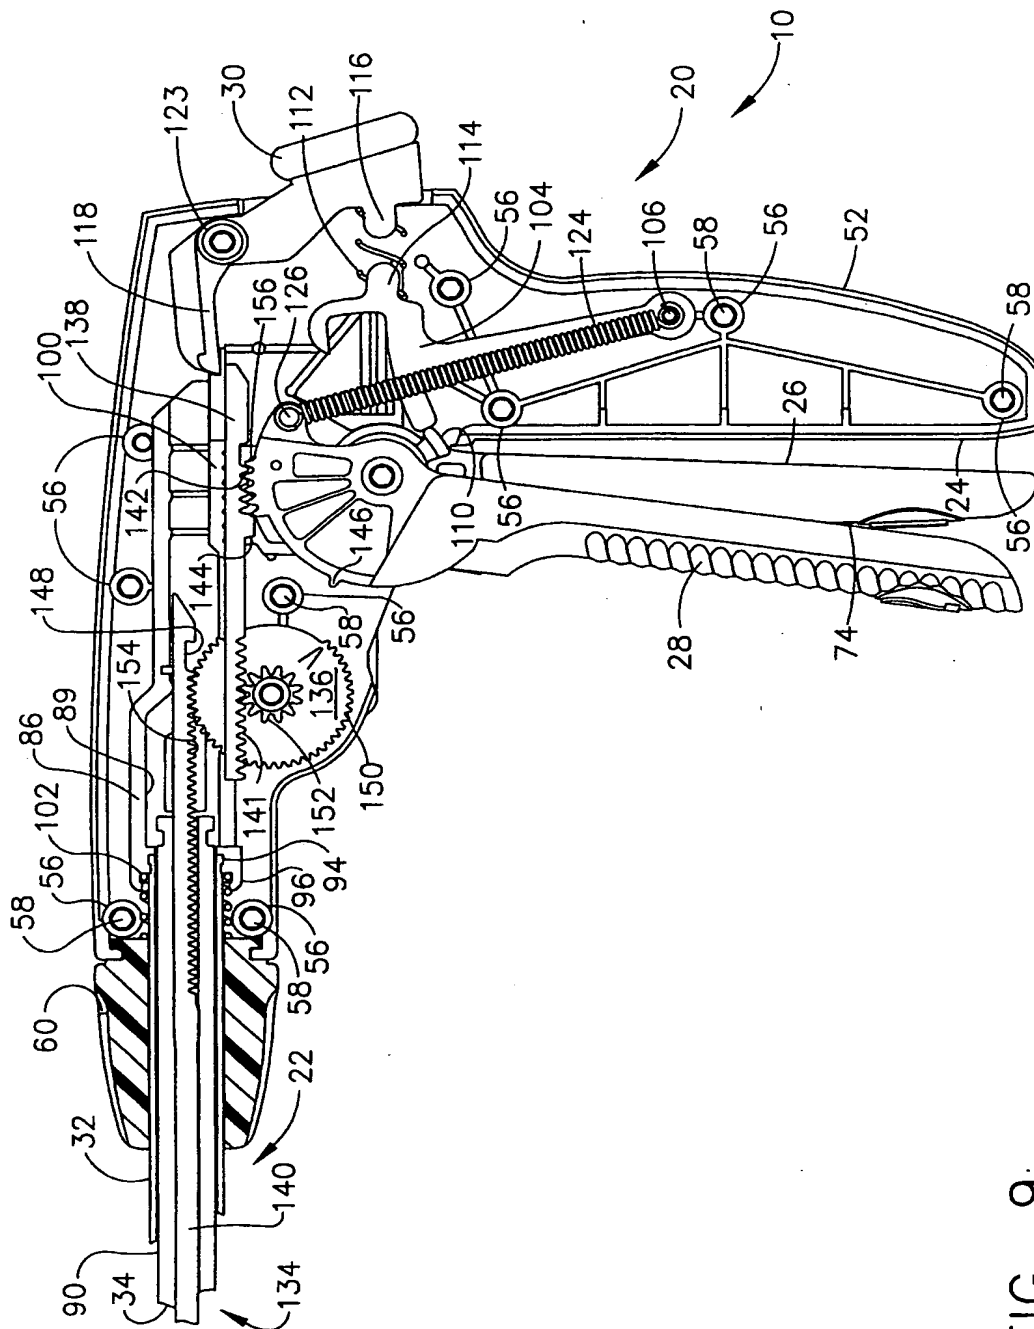


FIG. 9

8/27




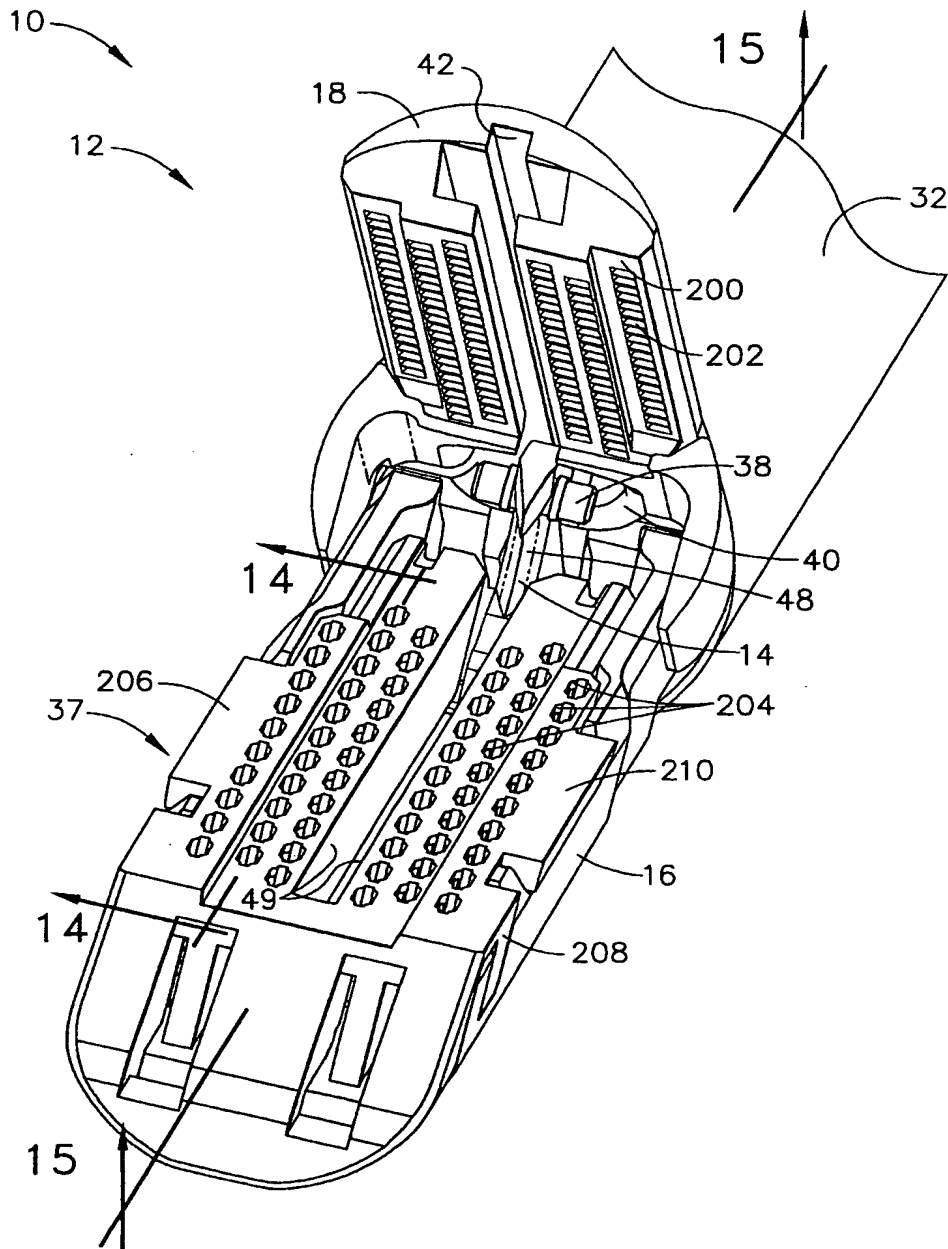

ATTY: Dean L. Garner: Phone: (513) 337-8559

FIG. 11

10/27

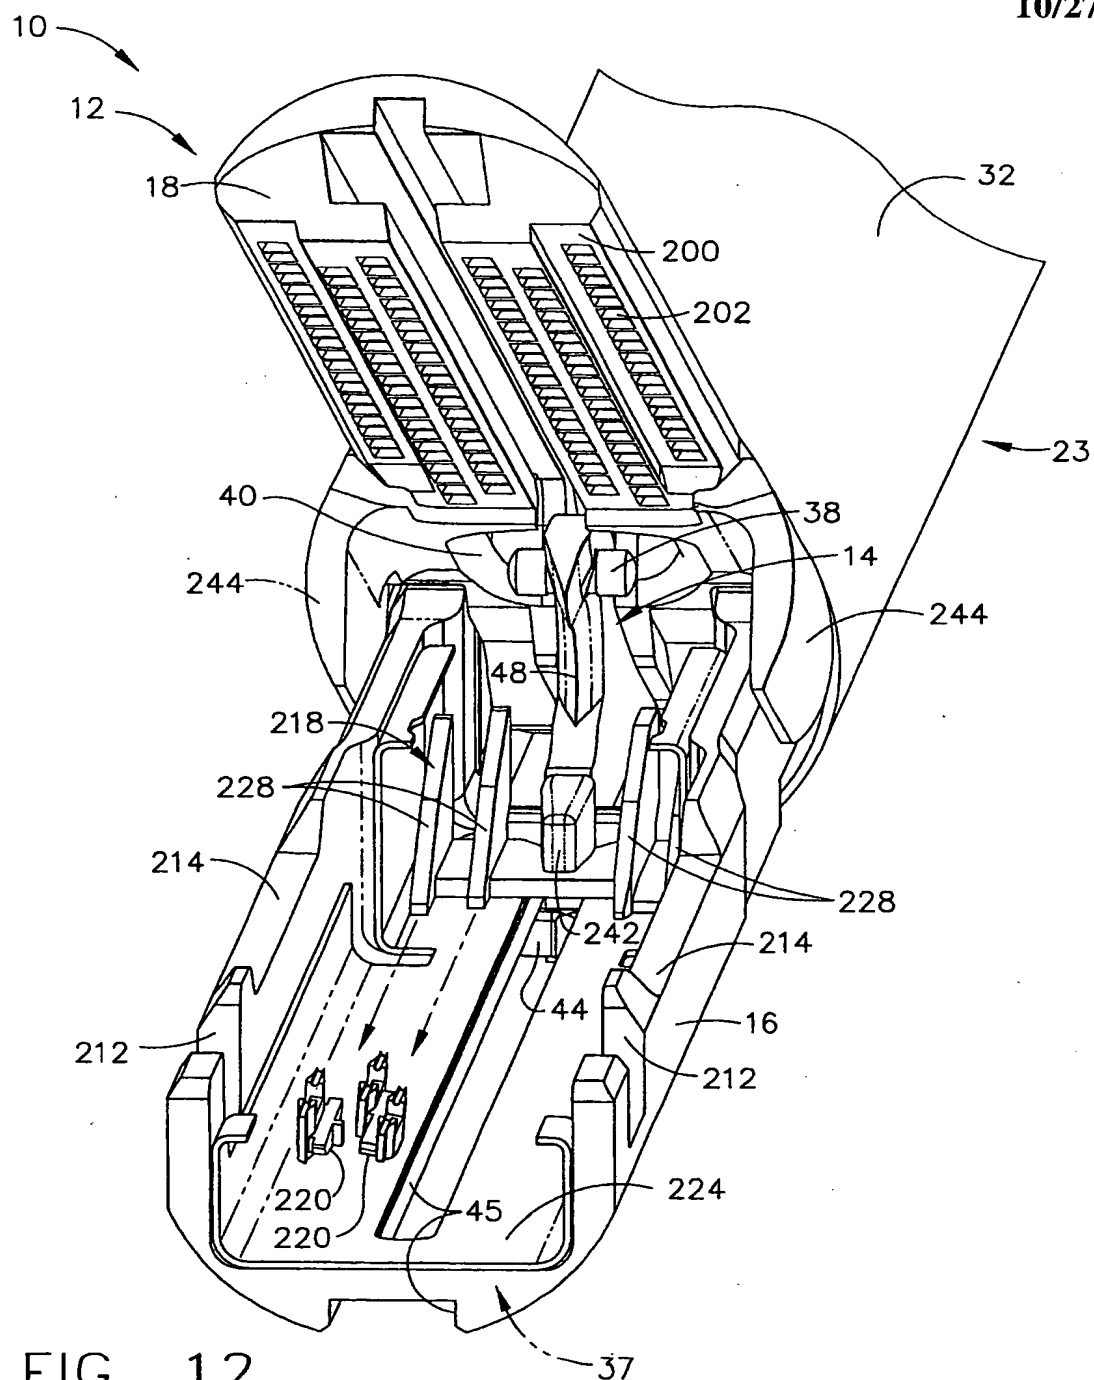

11/27


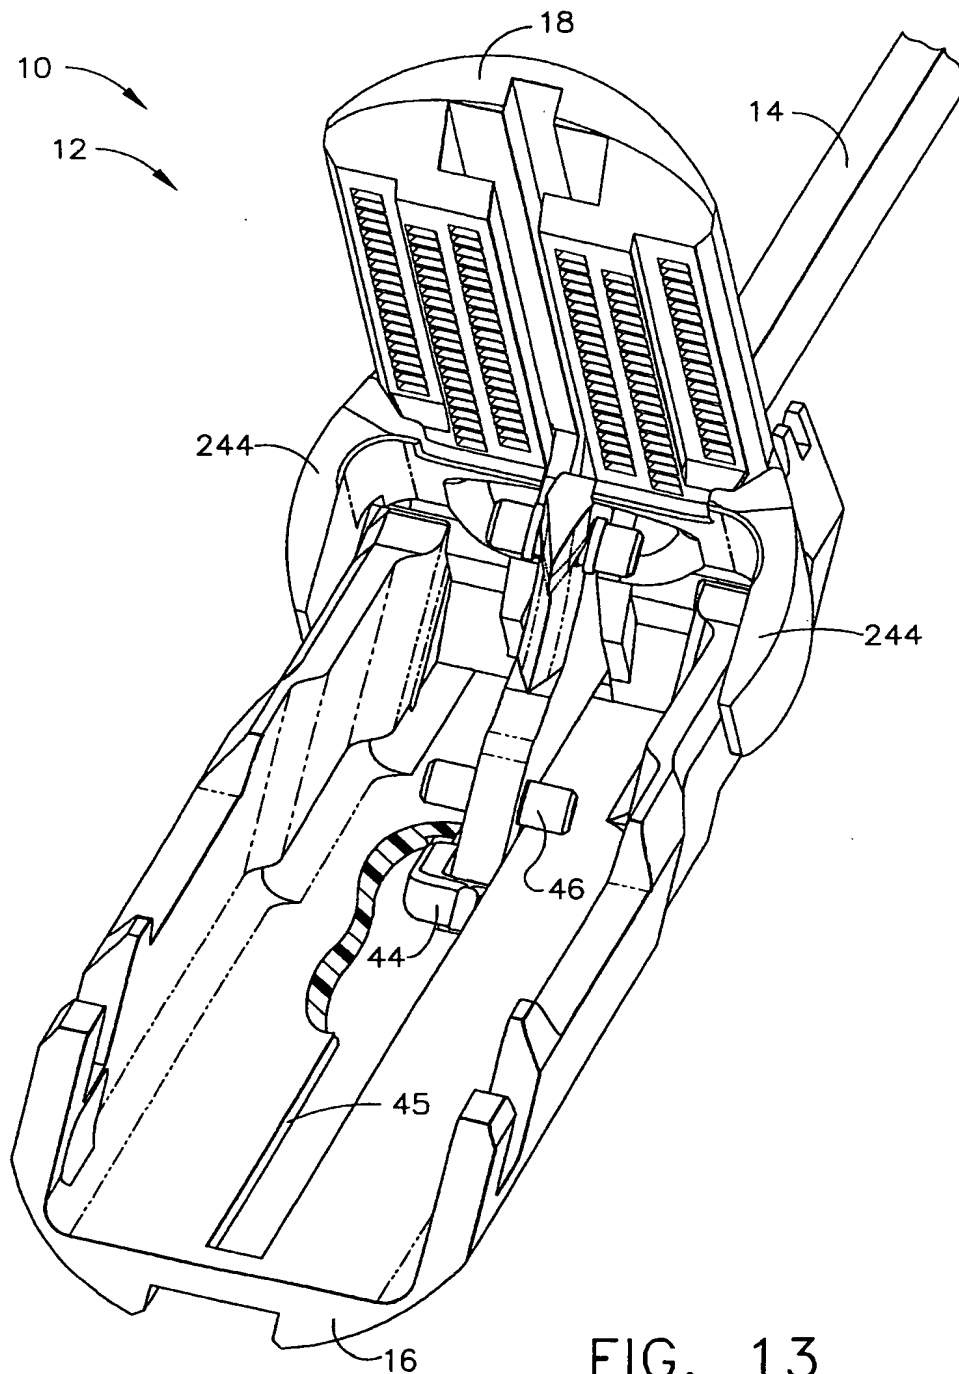


FIG. 13

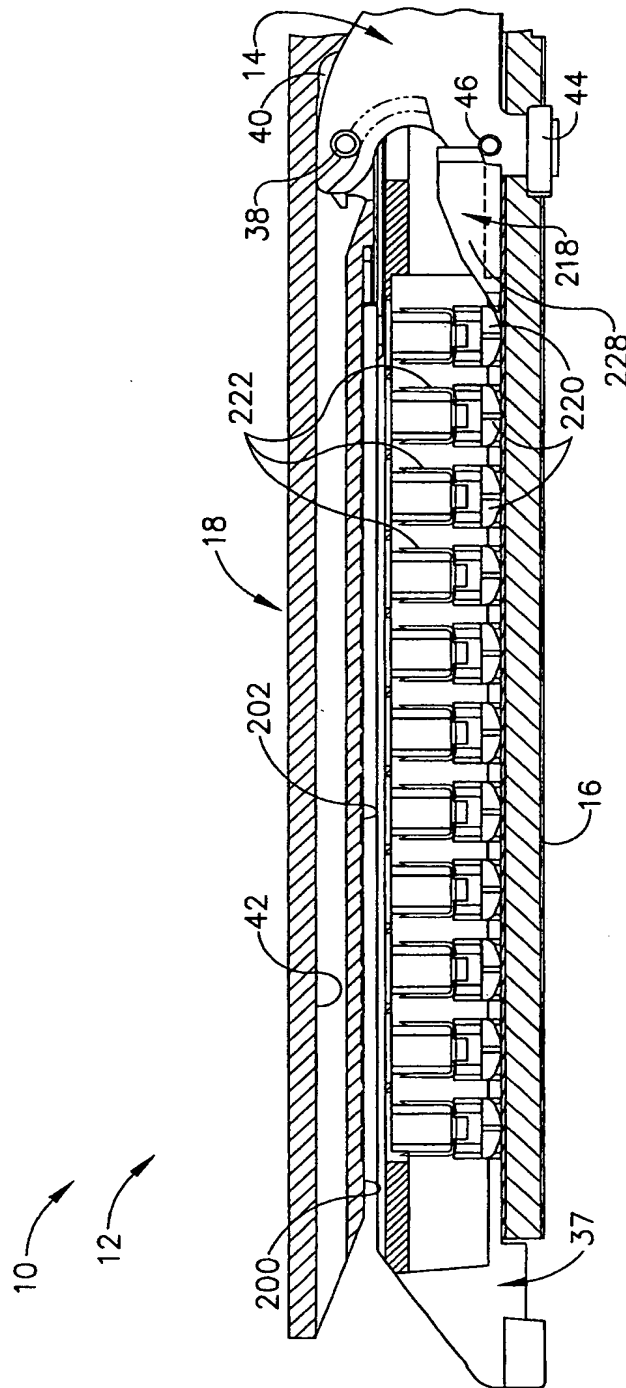

12/27

FIG. 14

13/27

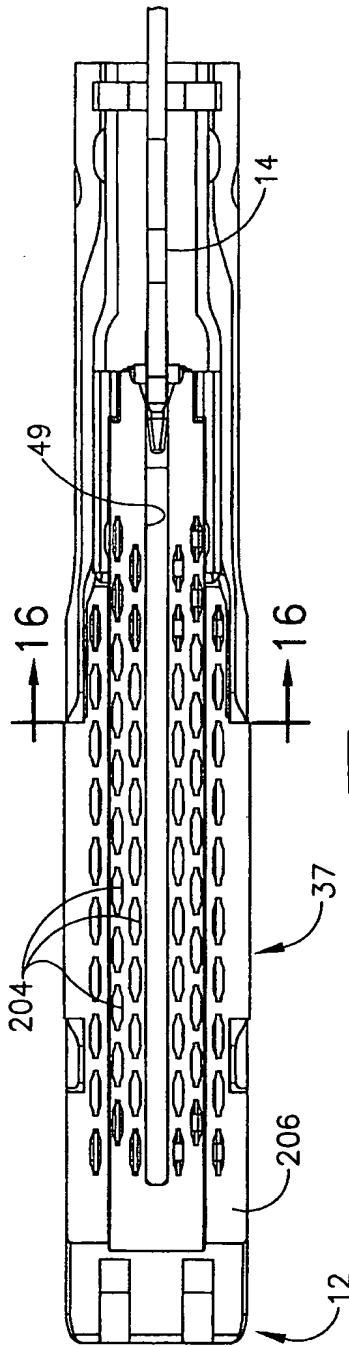


FIG. 15

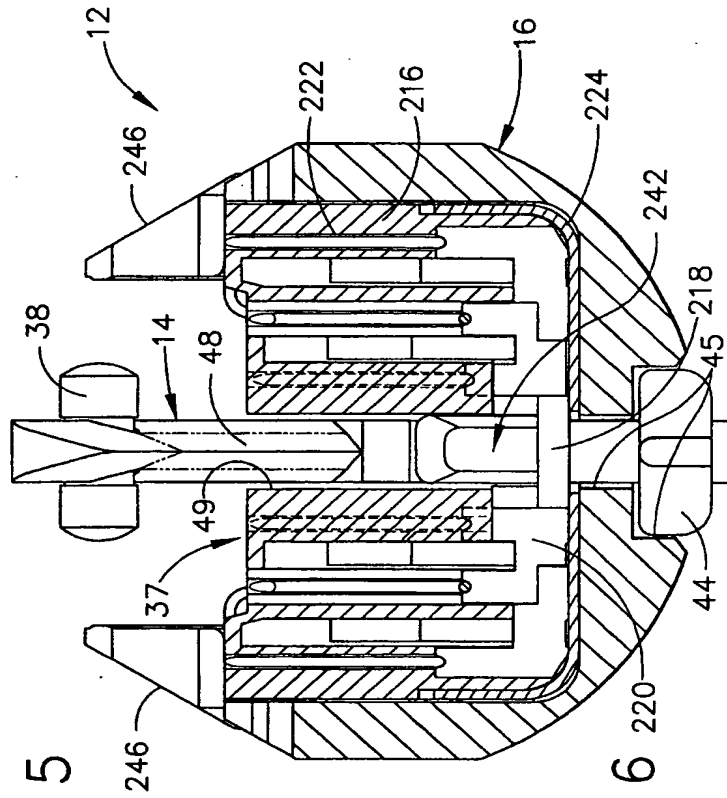


FIG. 16

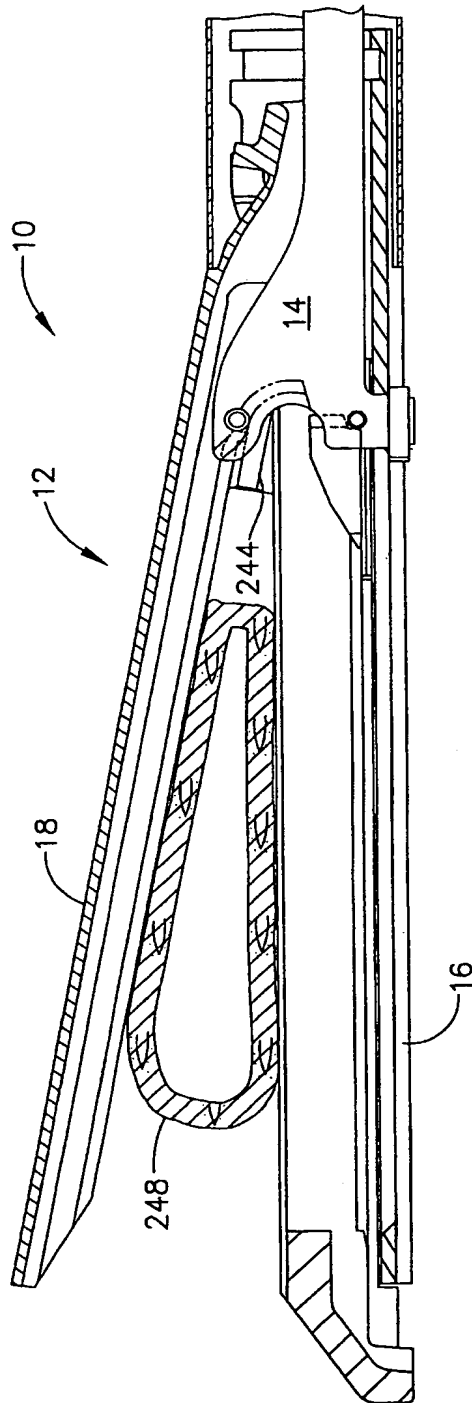


FIG. 17

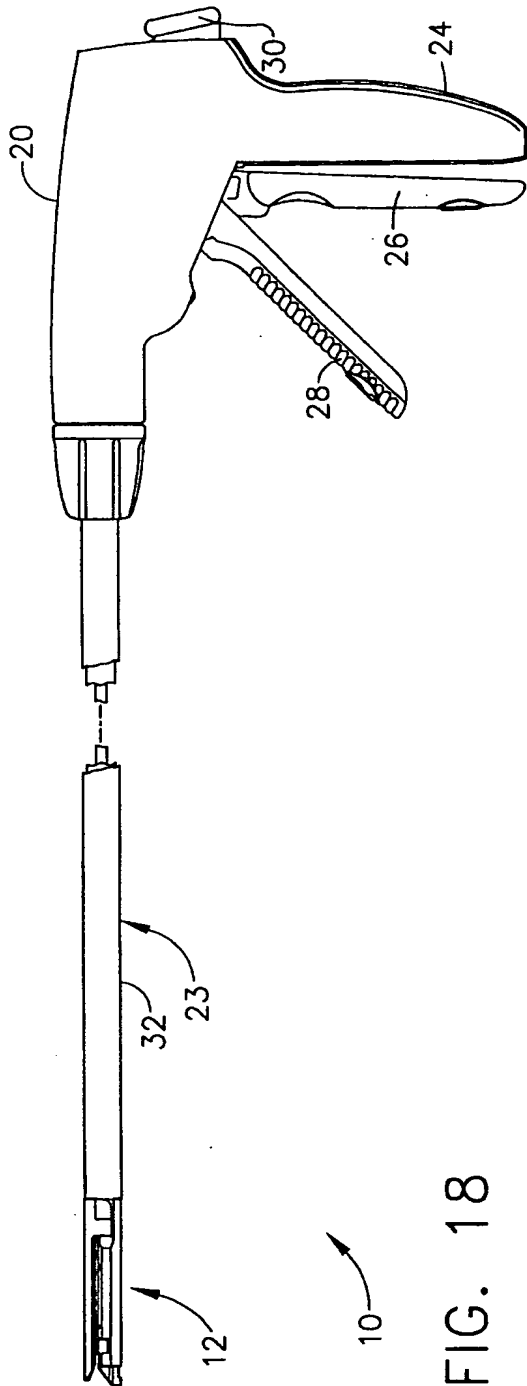


FIG. 18


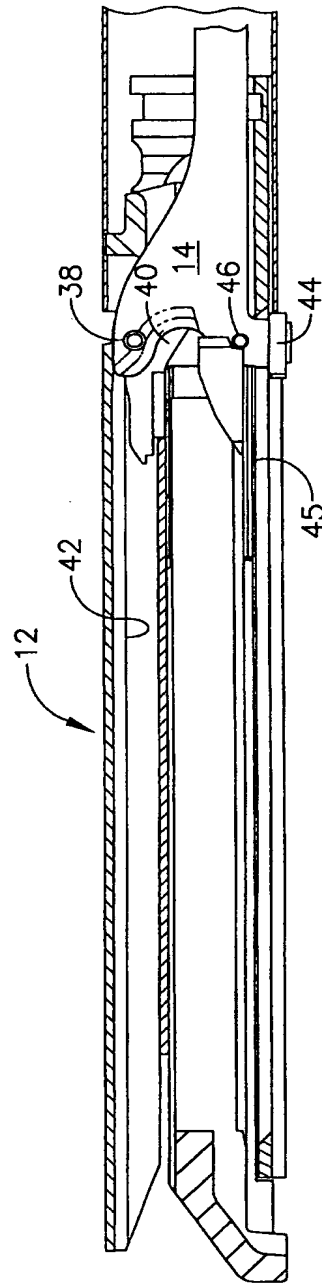


FIG. 19





17/27

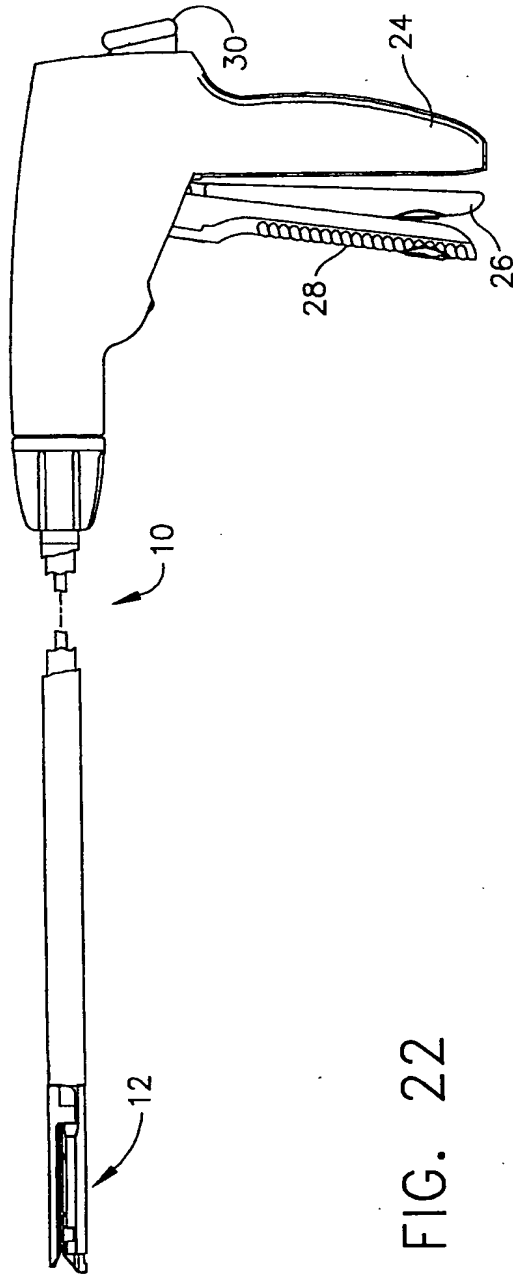


FIG. 22

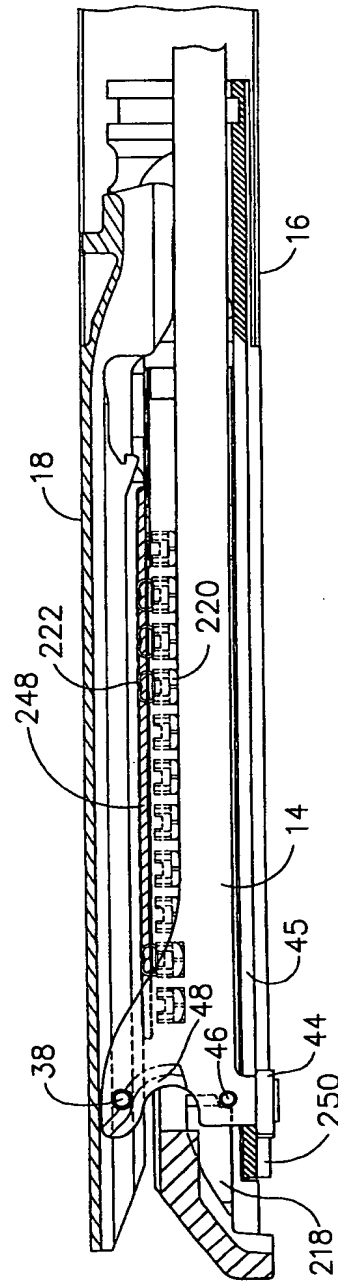


FIG. 23

18/27






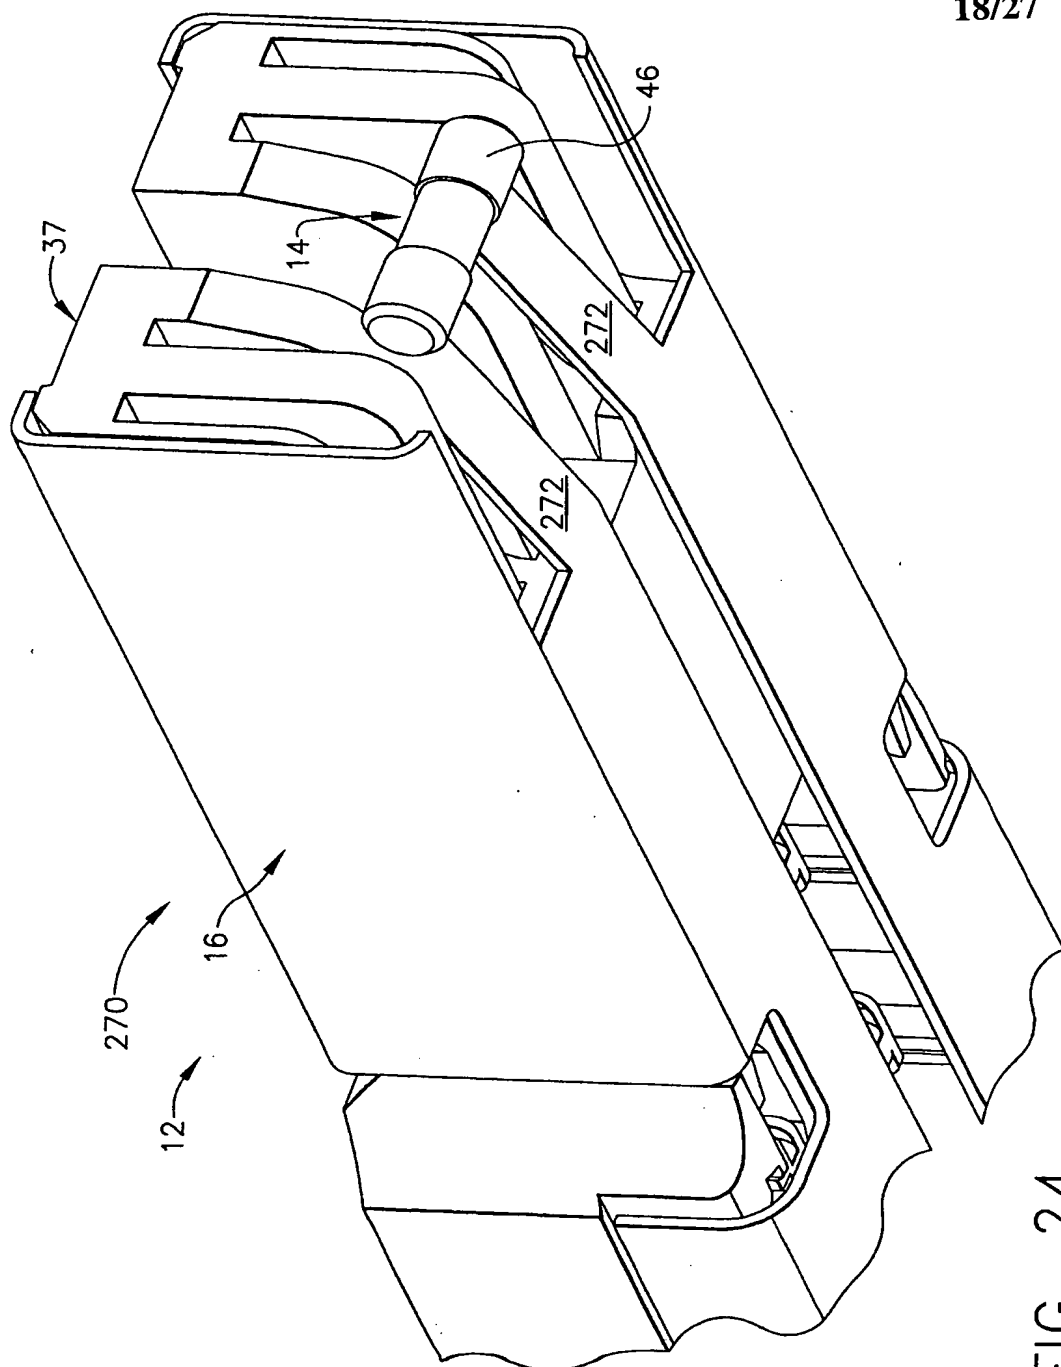



FIG. 24

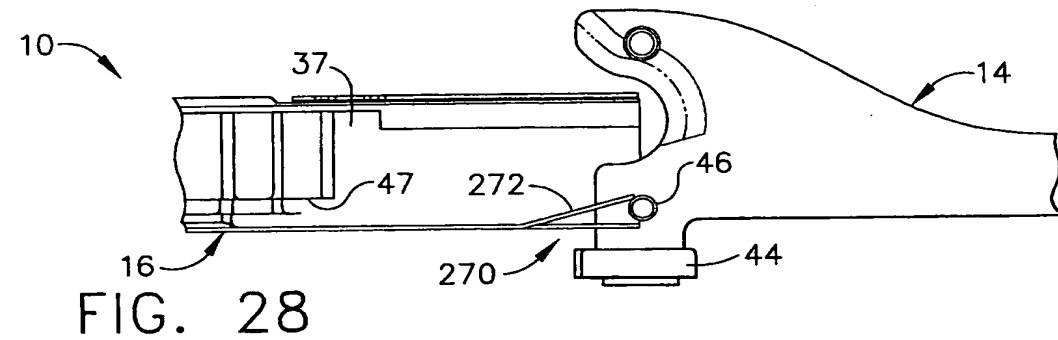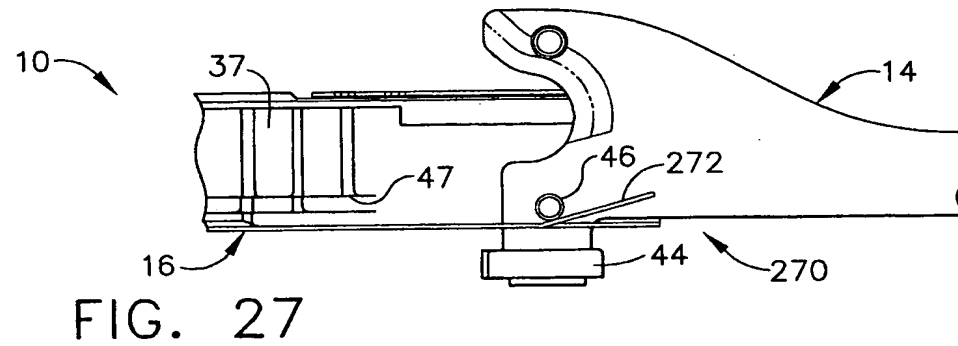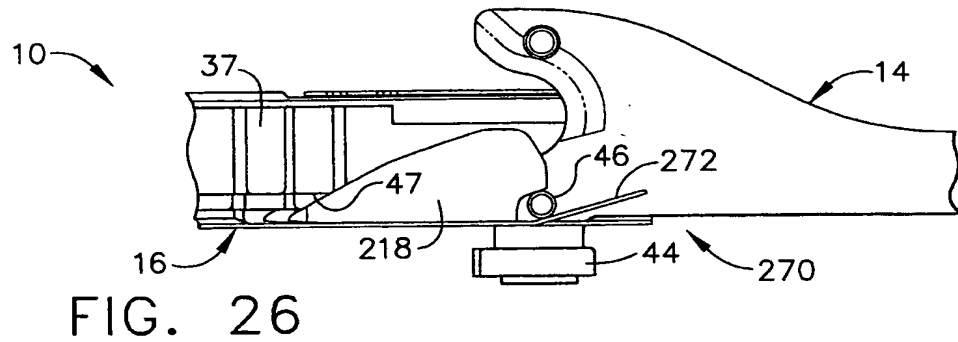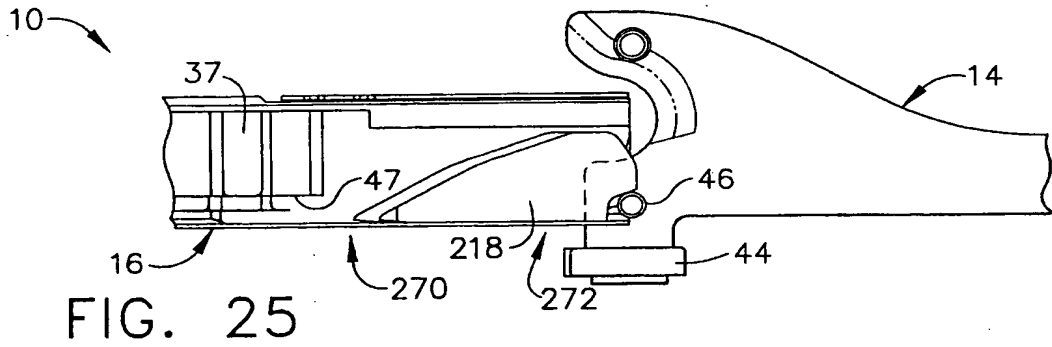

**20/27**

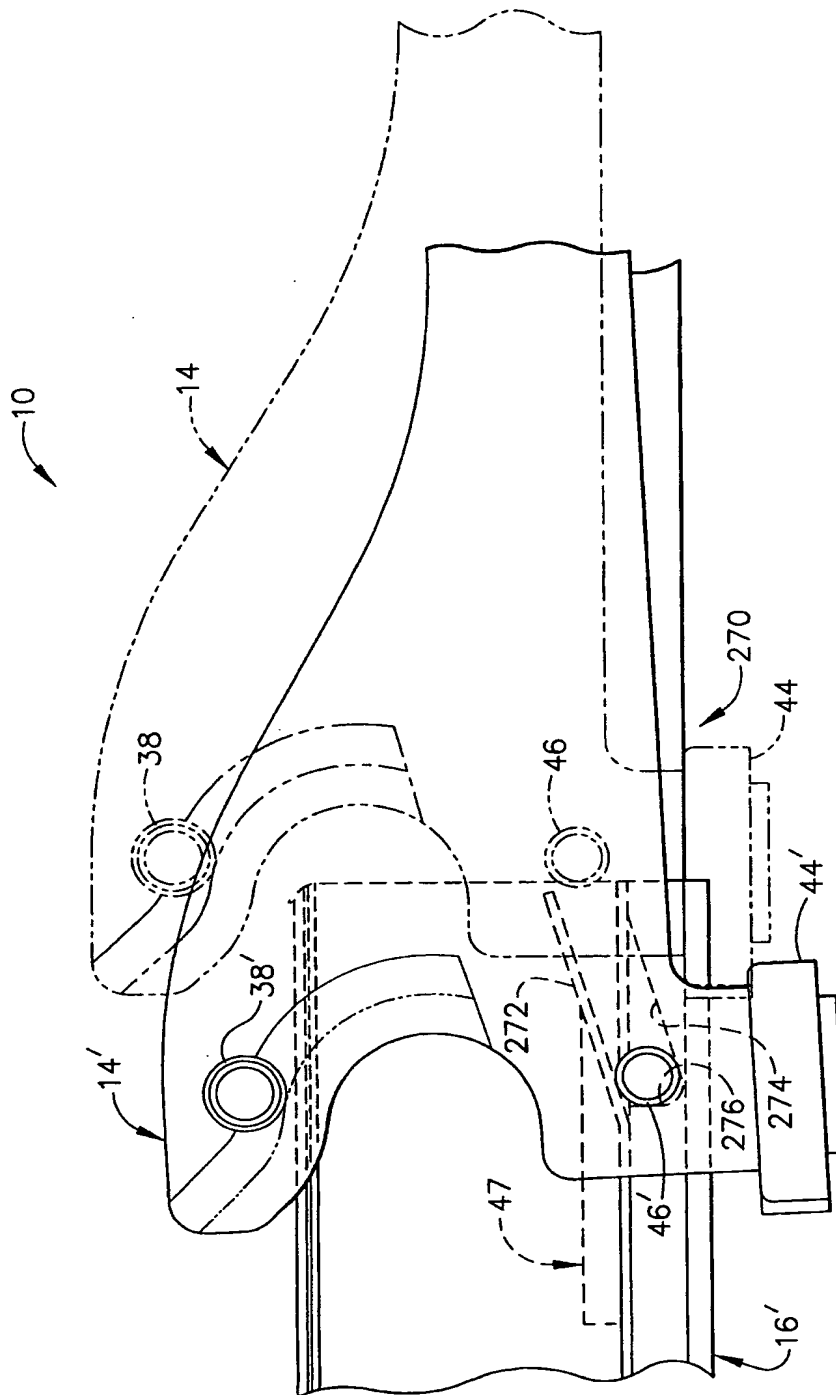

21/27

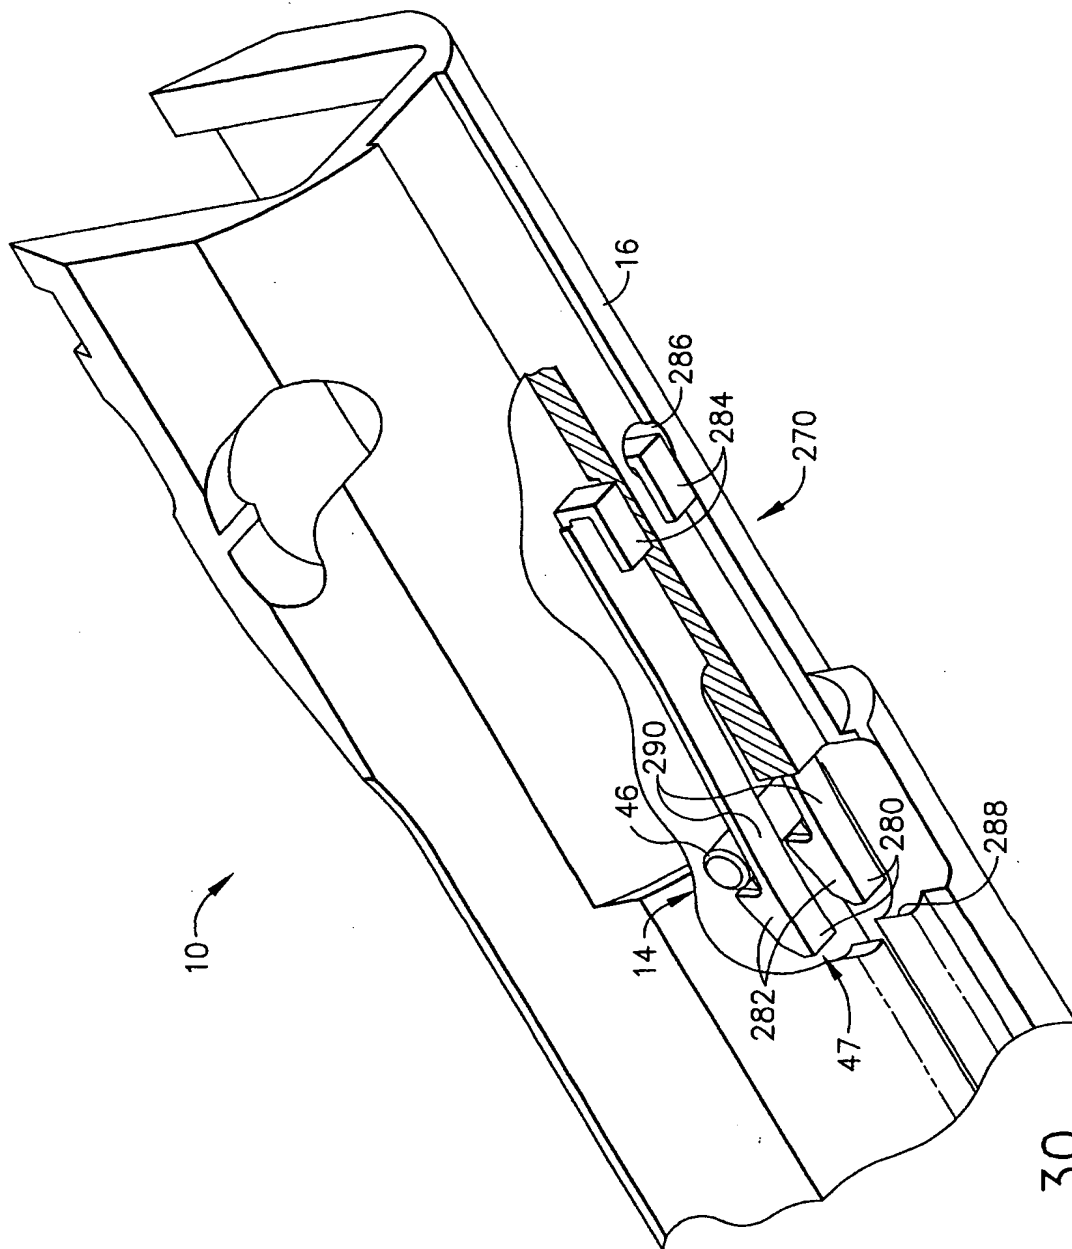

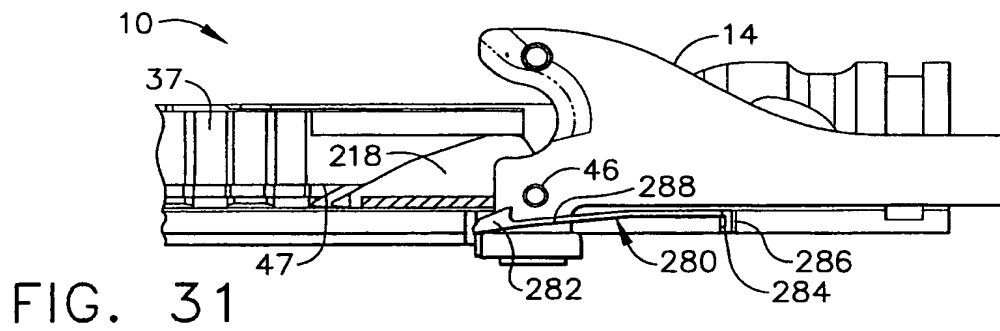


FIG. 31

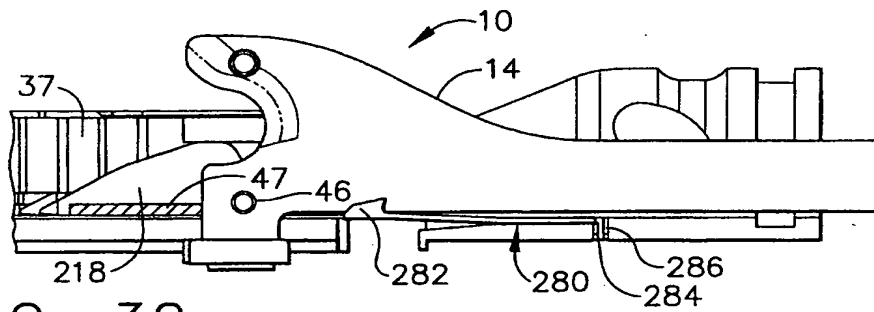


FIG. 32

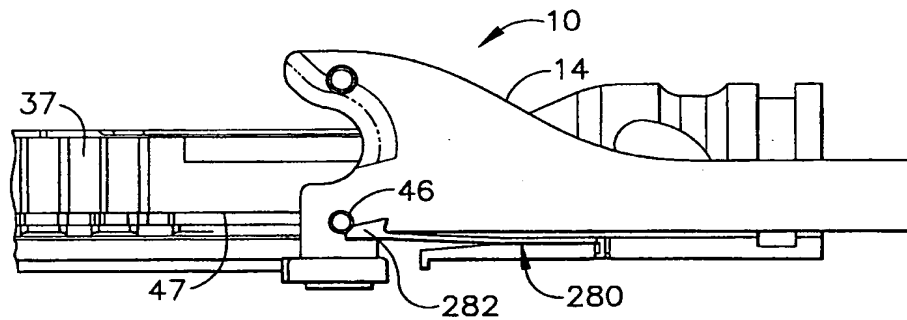


FIG. 33

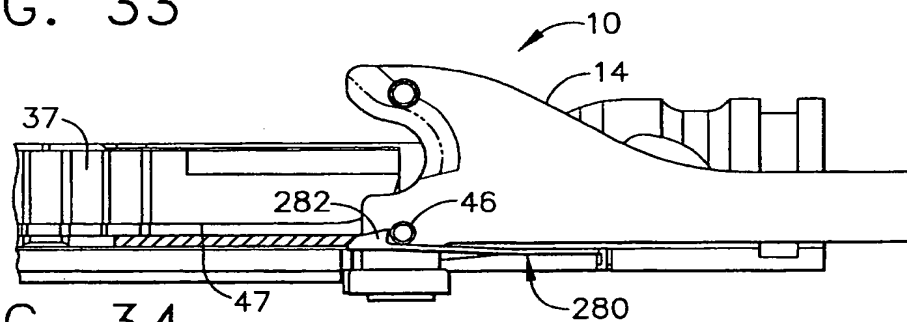


FIG. 34

23/27


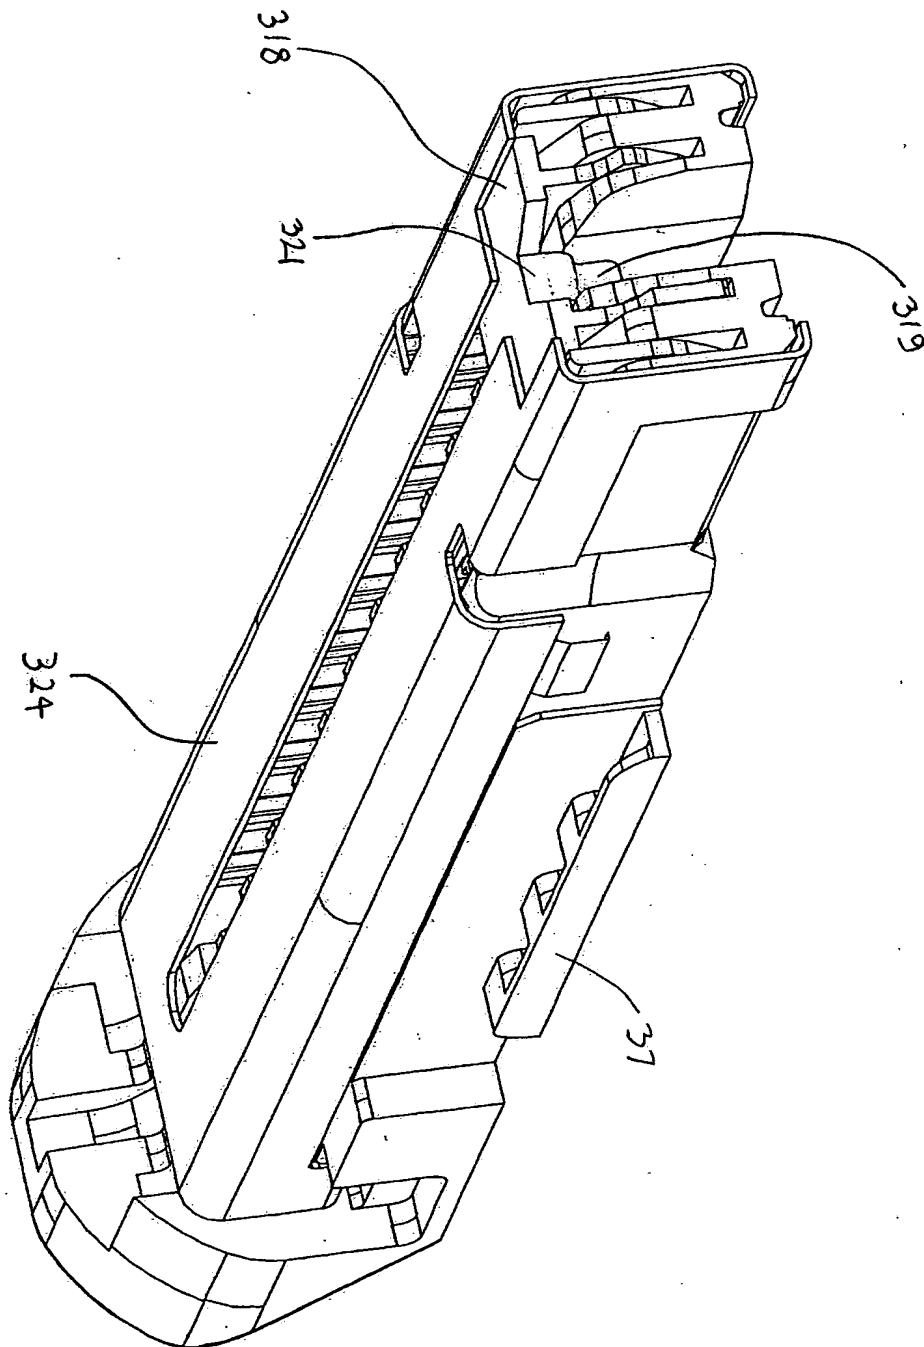


FIG. 35


24/27

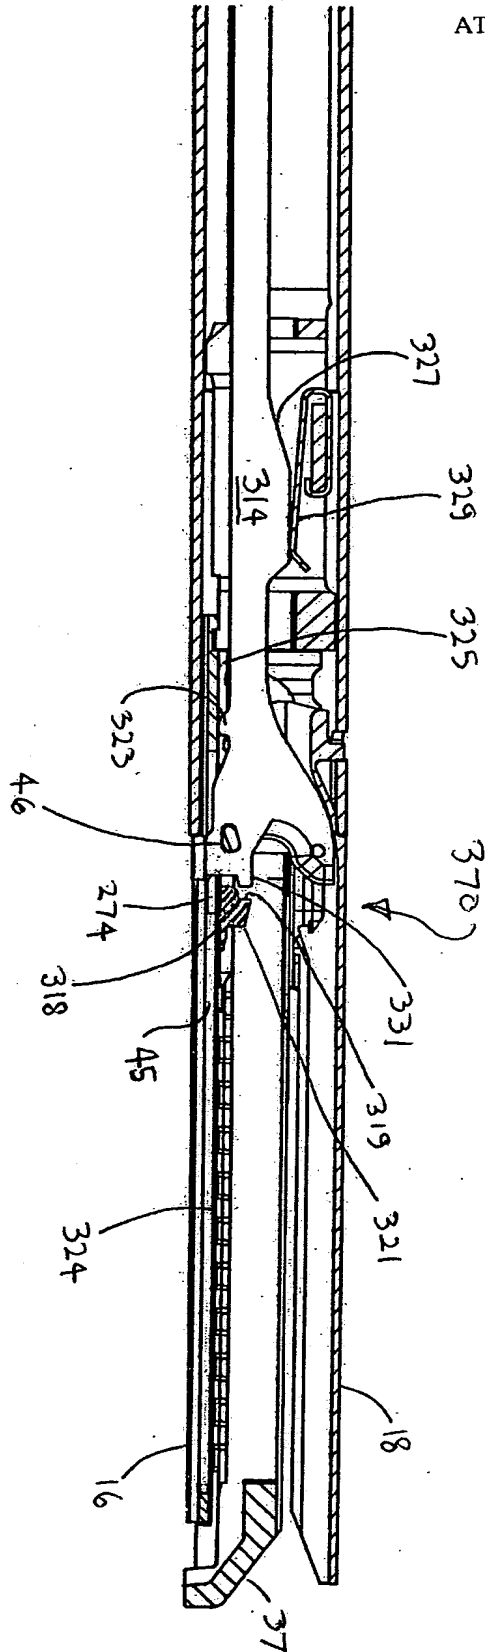

12


FIG. 36



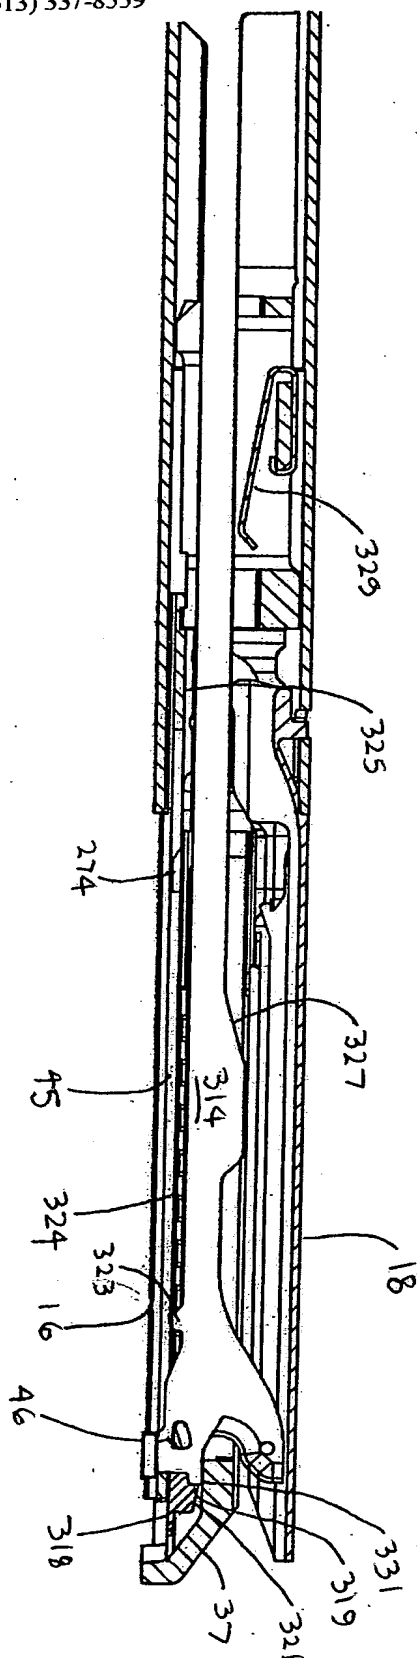

FI 6.37

26/27

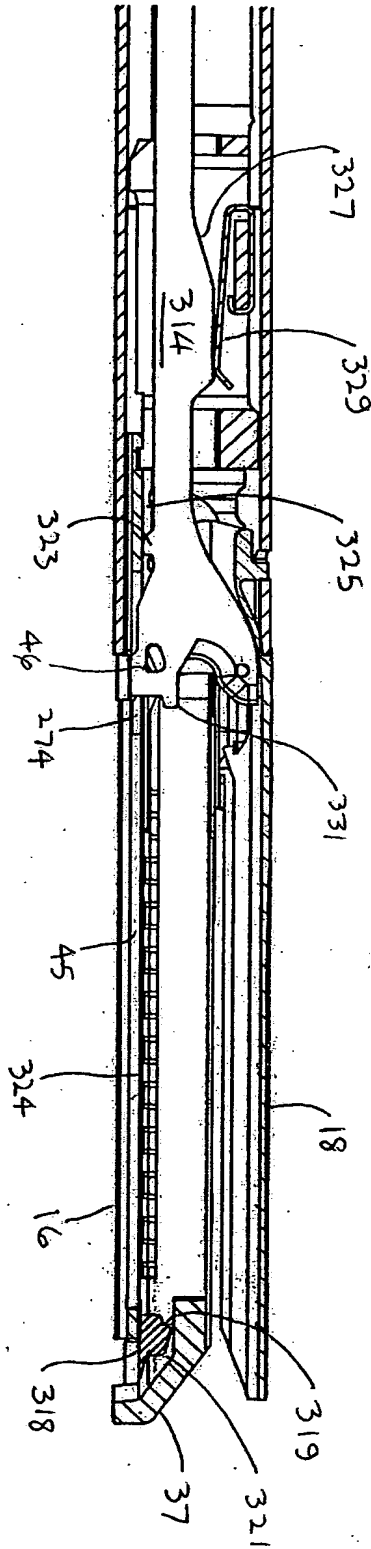

12

FIG. 38

ATTY: Dean L. Garner: Phone: (513) 337-8559

39

